



# Malachite Green Phosphate Assay Kit

## User Manual

Catalog # ASK1112

Detection and Quantification of Phosphate content in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

Bioworld Technology, Inc. (USA)

Email: [info@bioworld.com](mailto:info@bioworld.com)

Web: [www.bioworld.com](http://www.bioworld.com)

Bioworld technology, co. Ltd. (China)

Email: [info@biogot.com](mailto:info@biogot.com)

Web: [www.biogot.com](http://www.biogot.com)



I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....3

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7



**I. INTRODUCTION**

Malachite Green Phosphate Assay Kit provides a fast, reproducible, and non-radioactive method for measuring inorganic free phosphate in aqueous solutions. This simple assay method is based on the complex formed between malachite green molybdate and free orthophosphate under acidic conditions. The formation of the green molybdophosphoric acid complex measured at 635 nm is directly related to the free organic phosphate concentration. Applications for this assay include quantification of phosphorylation and phosphate release from protein phosphatase substrates. This assay measures only inorganic free phosphate; lipid-bound or protein-bound phosphates must first be hydrolyzed and neutralized prior to measurement. Overall, this assay is a reliable and suitable means of detecting and quantifying minimal amounts of inorganic free phosphate in acidic environments and is amenable to high-throughput screening applications.

**II. KIT COMPONENTS**

| Component              | Volume     | Storage            |
|------------------------|------------|--------------------|
| 96-Well Microplate     | 1 plate    |                    |
| Assay Buffer           | 30 ml x 4  | 4 °C               |
| Dye Reagent I          | 4 ml x 1   | 4 °C, keep in dark |
| Dye Reagent II         | Powder x 1 | 4 °C               |
| Dye Reagent II Diluent | 6 ml x 1   | 4 °C               |
| Standard (50 µmol/L)   | 1 ml x 1   | 4 °C               |
| Technical Manual       | 1 Manual   |                    |

**Note:**

**Dye Reagent II:** add 6 ml Dye Reagent II Diluent and heat to dissolve before use, store at 4 °C.

**III. MATERIALS REQUIRED BUT NOT PROVIDED**

1. Microplate reader to read absorbance at 635 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice



**IV. SAMPLE PREPARATION**

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 10,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 12,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For liquid samples

Detect directly.



**V. ASSAY PROCEDURE**

Add following reagents into the microplate:

| <b>Reagent</b>   | <b>Sample</b> | <b>Standard</b> | <b>Blank</b> |
|--|---------------|-----------------|--------------|
| Dye Reagent I  | 40 µl         | 40 µl           | 40 µl        |
| Dye Reagent II   | 60 µl         | 60 µl           | 60 µl        |
| Mix well.  |               |                 |              |
| Sample   | 100 µl        | --              |              |
| Standard   | --            | 100 µl          | --           |
| Distilled water  | --            | --              | 100 µl       |
| Mix, wait for 2 minutes, measured at 635 nm and record the absorbance. |               |                 |              |

**VI. CALCULATION**

1. According to the protein concentration of sample

$$\begin{aligned}\text{Phosphate } (\mu\text{mol/mg}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \\ &\quad / (V_{\text{Sample}} \times C_{\text{Protein}}) \\ &= 0.05 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}}\end{aligned}$$

2. According to the weight of sample

$$\begin{aligned}\text{Phosphate } (\mu\text{mol/g}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times W / V_{\text{Assay}}) \\ &= 0.05 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W\end{aligned}$$

3. According to the quantity of cells or bacteria

$$\begin{aligned}\text{Phosphate } (\mu\text{mol}/10^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \\ &\quad \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times N / V_{\text{Assay}}) \\ &= 0.05 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N\end{aligned}$$

4. According to the volume of sample

$$\begin{aligned}\text{Phosphate } (\mu\text{mol/ml}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \\ &\quad / V_{\text{Sample}} \\ &= 0.05 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}})\end{aligned}$$

$C_{\text{Protein}}$ : the protein concentration, mg/ml;

$C_{\text{Standard}}$ : the protein concentration, 50  $\mu\text{mol/L}$  = 0.05  $\mu\text{mol/ml}$ ;

$W$ : the weight of sample, g;

$N$ : the quantity of cell or bacteria,  $N \times 10^4$ ;


$V_{\text{Standard}}$ : the total volume of the reaction, 0.1 ml;

$V_{\text{Sample}}$ : the volume of sample, 0.1 ml;

$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml.

**VII. TYPICAL DATA**

The standard curve is for demonstration only. A standard curve must be run with each assay.

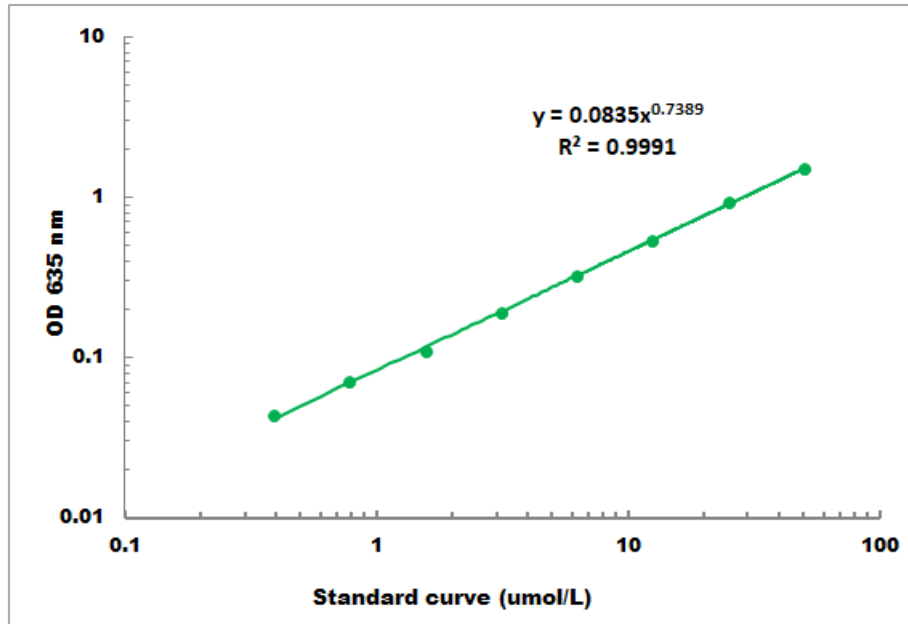

Detection Range: 1  $\mu\text{mol/L}$  - 50  $\mu\text{mol/L}$