



# Albumin (BCG) Microplate Assay Kit

## User Manual

Catalog # ASK1150

Detection and Quantification of Albumin Content in Urine, Serum,  
Plasma, Other biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

Bioworld Technology, Inc. (USA)

Email: [info@bioworld.com](mailto:info@bioworld.com)

Web: [www.bioworld.com](http://www.bioworld.com)

Bioworld technology, co. Ltd. (China)

Email: [info@biogot.com](mailto:info@biogot.com)

Web: [www.biogot.com](http://www.biogot.com)



I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....3

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7



**I. INTRODUCTION**

Albumin is the most abundant plasma protein in human. It accounts for about 60% of the total serum protein. Albumin plays important physiological roles, including maintenance of colloid osmotic pressure, binding of key substances such as long-chain fatty acids, bile acids, bilirubin, haematin, calcium and magnesium. It has anti-oxidant and anticoagulant effects, and also acts as a carrier for nutritional factors and drugs, as an effective plasma pH buffer. Serum albumin is a reliable prognostic indicator for morbidity and mortality, liver disease, nephritic syndrome, malnutrition and protein-losing enteropathies. High levels are associated with dehydration.

Albumin (BCG) Microplate Assay Kit is designed to measure albumin directly in biological samples without any pretreatment. The improved method utilizes bromocresol green that forms a colored complex specifically with albumin. The intensity of the color, measured at 630nm, is directly proportional to the albumin concentration in the sample.



II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Dye Reagent	Powder x 1	4 °C
Standard	Powder x 1	-20 °C
Technical Manual	1 Manual	

**Note:**

**Dye Reagent:** add 20 ml distilled water to dissolve before use. Store diluted standards at 4 °C.

**Standard:** add 0.5 ml distilled water to dissolve, the concentration will be 100 mg/ml. Store diluted standards at -20 °C.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 630 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Centrifuge
6. Timer



---

**IV. SAMPLE PREPARATION**

1. For serum, plasma or blood samples

Dilute serum and plasma samples with distilled water, then detect directly.



**V. ASSAY PROCEDURE**

Add following reagents in the microcentrifuge tube:

<b>Reagent</b>	<b>Sample</b>	<b>Standard</b>	<b>Blank</b>
Sample	2 $\mu$ l	--	--
Standard	--	2 $\mu$ l	--
Distilled water		--	2 $\mu$ l
Dye Reagent	200 $\mu$ l	200 $\mu$ l	200 $\mu$ l
Mix, incubate 5 min at room temperature, record absorbance measured at 630 nm.			



VI. CALCULATION

1. According to the volume of sample

$$\begin{aligned} \text{Albumin (mg/ml)} &= C_{\text{Standard}} \times V_{\text{Standard}} \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &V_{\text{Sample}} \\ &= 100 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$


C<sub>Standard</sub>: the standard concentration, 100 mg/ml;

V<sub>Standard</sub>: the volume of standard, 0.002 ml;

V<sub>Sample</sub>: the volume of sample, 0.002 ml.

**VII. TYPICAL DATA**

The standard curve is for demonstration only. A standard curve must be run with each assay.

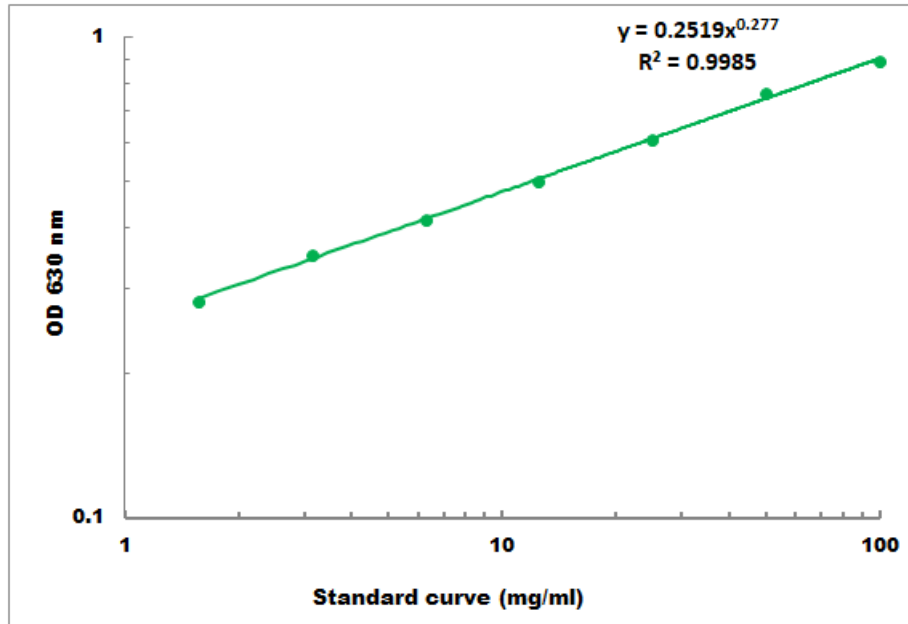

Detection Range: 1 mg/ml - 100 mg/ml