



# Amylopectin Microplate Assay Kit

## User Manual

Catalog # ASK1179

Detection and Quantification of Amylopectin content in Tissue extracts, Other biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

Bioworld Technology, Inc. (USA)

Email: [info@bioworld.com](mailto:info@bioworld.com)

Web: [www.bioworld.com](http://www.bioworld.com)

Bioworld technology, co. Ltd. (China)

Email: [info@biogot.com](mailto:info@biogot.com)

Web: [www.biogot.com](http://www.biogot.com)



I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....3

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7



## **I. INTRODUCTION**

Amylopectin is a water-soluble polysaccharide and highly branched polymer of  $\alpha$ -glucose units found in plants. It is one of the two components of starch, the other being amylose.

Amylopectin Microplate Assay Kit is a sensitive assay for determining amylopectin content in various samples. The purplish red is produced according to the action of amylopectin and iodine reagent. The measurement wavelength and reference wavelength of the amylose were 550nm and 735 nm. The absorbance difference between the two wavelengths is directly proportional to the content.



II. KIT COMPONENTS

| Component          | Volume     | Storage            |
|--------------------|------------|--------------------|
| 96-Well Microplate | 1 plate    |                    |
| Assay Buffer       | 30 ml x 4  | 4 °C               |
| Reaction Buffer A  | 10 ml x 1  | 4 °C               |
| Reaction Buffer B  | 8 ml x 1   | 4 °C               |
| Dye Reagent        | 1 ml x 1   | 4 °C, keep in dark |
| Standard           | Powder x 1 | 4 °C               |
| Technical Manual   | 1 Manual   |                    |

**Note:**

**Standard:** add 1 ml Assay Buffer to dissolve before use, the concentration will be 4 mg/ml.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 550nm and 735 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Centrifuge
6. Timer
7. Mortar



---

**IV. SAMPLE PREPARATION**

1. For Tissue samples

Weigh out 0.01 g tissue, homogenize with 1 ml Assay buffer, then transfer all the lysate to the microtube, centrifuged at 4000g for 10 minutes; take the supernatant into a new centrifuge tube for detection.



**V. ASSAY PROCEDURE**

Add following reagents into the microplate:

| <b>Reagent</b>  | <b>Sample</b> | <b>Standard</b> | <b>Blank</b> |
|---|---------------|-----------------|--------------|
| Sample  | 10 µl         | --              | --           |
| Standard  | --            | 10 µl           | --           |
| Distilled water   | --            | --              | 10 µl        |
| Reaction Buffer A   | 100 µl        | 100 µl          | 100 µl       |
| Reaction Buffer B   | 80 µl         | 80 µl           | 80 µl        |
| Dye Reagent   | 10 µl         | 10 µl           | 10 µl        |
| Mix, wait for 5 minutes, record absorbance measured at 550nm and 735nm. |               |                 |              |

**VI. CALCULATION**

1. According to the volume of sample

$$\begin{aligned} \text{Amylopectin (mg/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times [(OD_{\text{Sample550}} - OD_{\text{Sample735}}) - OD_{\text{Blank}}] / \\ & \quad [(OD_{\text{Standard550}} - OD_{\text{Standard735}}) - OD_{\text{Blank}}] / V_{\text{Sample}} \\ &= 4 \times [(OD_{\text{Sample550}} - OD_{\text{Sample735}}) - OD_{\text{Blank}}] / [(OD_{\text{Standard550}} - \\ & \quad OD_{\text{Standard735}}) - OD_{\text{Blank}}] \end{aligned}$$

2. According to the weight of sample

$$\begin{aligned} \text{Amylopectin (mg/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times [(OD_{\text{Sample550}} - OD_{\text{Sample735}}) - OD_{\text{Blank}}] / \\ & \quad [(OD_{\text{Standard550}} - OD_{\text{Standard735}}) - OD_{\text{Blank}}] / (V_{\text{Sample}} \times W / V_{\text{Assay}}) \\ &= 4 \times [(OD_{\text{Sample550}} - OD_{\text{Sample735}}) - OD_{\text{Blank}}] / [(OD_{\text{Standard550}} - \\ & \quad OD_{\text{Standard735}}) - OD_{\text{Blank}}] / W \end{aligned}$$

$C_{\text{Standard}}$ : the standard concentration, 4 mg/ml;

$W$ : the weight of sample, g;


$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml

$V_{\text{Standard}}$ : the volume of standard, 10  $\mu$ l;

$V_{\text{Sample}}$ : the volume of sample, 10  $\mu$ l.

**VII. TYPICAL DATA**

The standard curve is for demonstration only. A standard curve must be run with each assay.

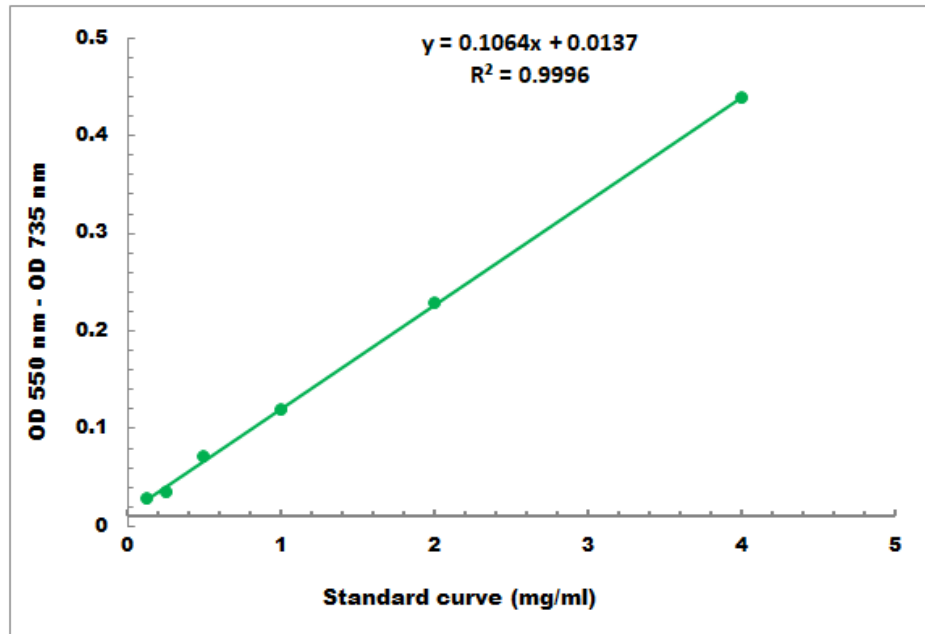

Detection Range: 0.1 mg/ml - 4 mg/ml