



Urease Microplate Assay Kit

User Manual

Catalog # ASK1180

Detection and Quantification of Urease activity in Urine, Tissue extracts, Cell lysate, Cell culture, Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.

Bioworld Technology, Inc. (USA)

Email: info@bioworld.com

Web: www.bioworld.com

Bioworld technology, co. Ltd. (China)

Email: info@biogot.com

Web: www.biogot.com



I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....3

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7



I. INTRODUCTION

Urease (Amidohydrolase, EC 3.5.1.5) is an enzyme that catalyzes the hydrolysis of urea into carbon dioxide and ammonia. Many gastrointestinal or urinary tract pathogens produce urease. Thus its activity is a useful diagnostic parameter for the presence of pathogens such as *Helicobacter pylori*. Urease is found in bacteria, yeast, and higher plants. Urease activity is commonly determined in anaerobes of the bovine rumen, human feces and environmental samples such as soils and phytoplanktons.

Urease Microplate Assay Kit provides a very sensitive and convenient means to measure urease activity in a variety of samples. In the assay, urease reacts with urea, resulting in the formation of ammonia, which is determined at 620nm, is directly proportional to the urease activity in the sample.

**II. KIT COMPONENTS**

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Substrate	Powder x 1	4 °C
Substrate Diluent	10 ml x 1	4 °C
Dye Reagent I	Powder x 1	4 °C
Dye Reagent II	5 ml x 1	4 °C
Standard	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

Note:

Substrate: add 10 ml Substrate Diluent to dissolve before use.

Dye Reagent I: add 4 ml distilled water to dissolve before use.

Standard: add 1 ml distilled water to dissolve, then add 25 µl to 975 µl distilled water, mix, the concentration will be 5 mmol/L.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 620 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer



IV. SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 10000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 10000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For urine and Other biological fluids media samples

Detect directly.

**V. ASSAY PROCEDURE**

Add following reagents in the microplate:

Reagent	Sample	Control	Standard	Blank
Substrate	100 μ l	100 μ l	--	--
Sample	10 μ l	--	--	--
Standard	--	--	10 μ l	--
Distilled water	--	10 μ l	100 μ l	110 μ l
Shake and mix, put it into the oven, 37 °C for 10 minutes.				
Dye Reagent I	40 μ l	40 μ l	40 μ l	40 μ l
Dye Reagent II	50 μ l	50 μ l	50 μ l	50 μ l
Shake and mix, put it into the oven, 37 °C for 15 minutes. Then record absorbance measured at 620 nm.				

VI. CALCULATION

Unit Definition: One unit of Urease activity is defined as the enzyme produces 1 μmol of ammonia per minute.

1. According to the volume of liquid sample

$$\begin{aligned}\text{Urease (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &V_{\text{Sample}} / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}})\end{aligned}$$

2. According to the weight of sample

$$\begin{aligned}\text{Urease (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (W \times \\ &V_{\text{Sample}} / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W\end{aligned}$$

3. According to the quantity of cell or bacteria

$$\begin{aligned}\text{Urease (U/10}^4\text{)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (N \times \\ &V_{\text{Sample}} / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N\end{aligned}$$

C_{Standard} : the concentration of Standard, 5 mmol/L = 5 $\mu\text{mol/ml}$;

W: the weight of sample, g;

N: the quantity of cell or bacteria, $N \times 10^4$;

V_{Standard} : the volume of standard, 0.01 ml;


V_{Sample} : the volume of sample, 0.01 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;

T: the reaction time, 10 minutes.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

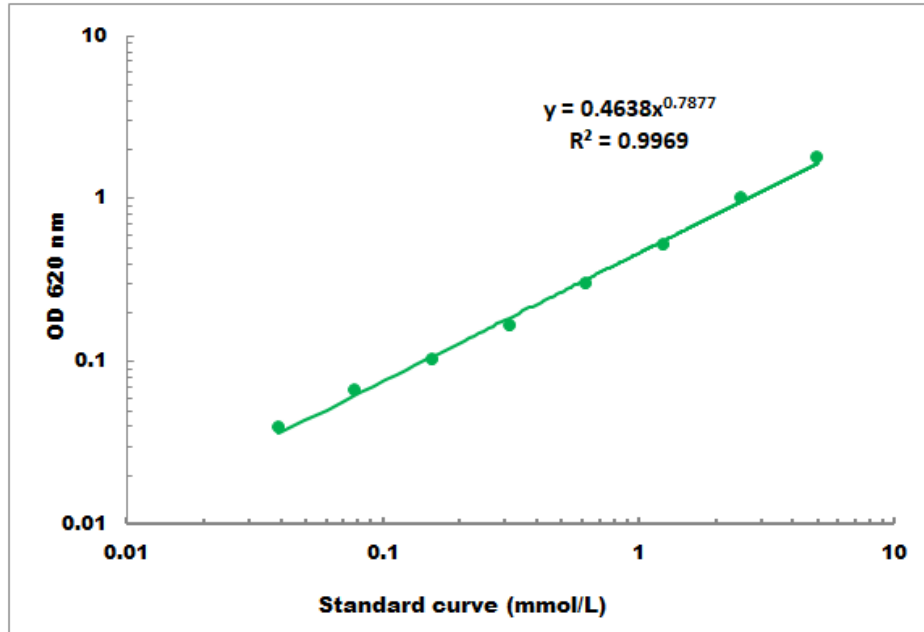

Detection Range: 0.05 mmol/L - 5 mmol/L